

Vernier Caliper, Depth Gage

**Vernier Caliper (standard and long-size)
Depth Gage**

Safety Precautions

To ensure operator safety, use this product in conformance with the directions, functions and specifications given in this User's Manual. Use under other conditions may compromise safety.

⚠ CAUTION Shows risks that could result in minor or moderate injury.

- The outside and inside measuring jaws of this caliper have sharp edges. Handle it with great care to avoid injury.
- Do not measure the workpiece if it is rotating. There is a risk of injury due to being caught in the machine, etc.

■ Conventions and wording indicating prohibited and mandatory actions



Indicates concrete information about prohibited actions.



Indicates concrete information about mandatory actions.

Contents

1	Type and Code Number	2
2	Names of Components	3
3	Product Applications	4
4	Precautions before Use	4
5	Basic Usage	5
6	Confirmation before Measurement	5
7	Measurement Meth	6
8	Reading Measurements	8
9	Precautions after Use	8

User's Manual

No. 99MAC002A1
Date of publication: May 1, 2023 (1)

1 Type and Code Number


■ Caliper: Standard



Code number

530-101 530-108 530-109 530-100
530-102 530-501 530-502 530-320
530-321 530-322 530-335

■ Caliper: Long-size

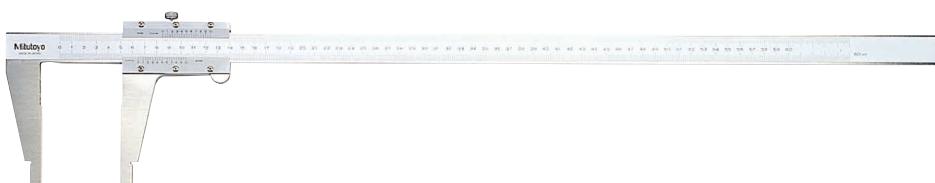

Code number

160-130 160-131 160-132 160-133 160-134

● With Fine-Adjustment



Code number

160-127 160-128 160-101 160-104
160-110 160-113

● With Fine-Adjustment



Code number

532-101 532-102 532-103

● With Automatic Clamp



Code number

531-101 531-102 531-103

● Long-jaw



Code number

534-109 534-110


● Long-jaw with Fine-Adjustment



Code number

534-113 534-114
534-115 534-116


■ Depth Gage

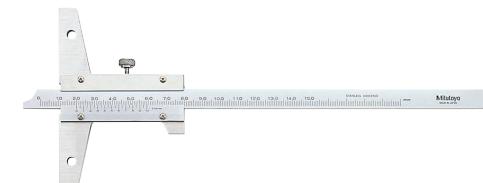

Code number

527-201 527-202 527-203 527-204
527-205


● Long-jaw

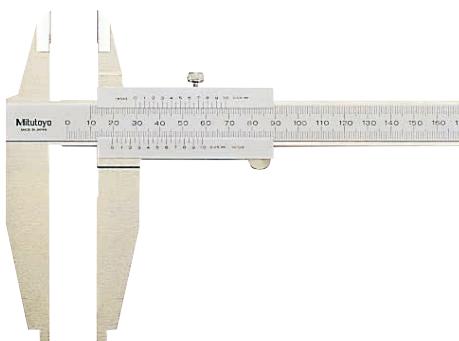

Code number

533-404 533-405 533-406


● Long-jaw with Fine-Adjustment

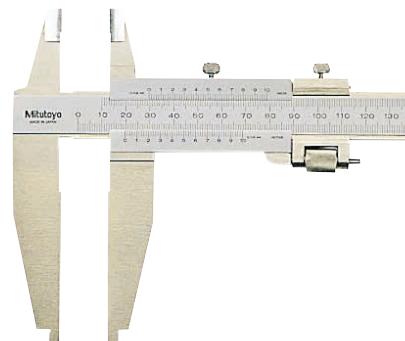

Code number

533-504 533-505 533-506

● With Fine-Adjustment

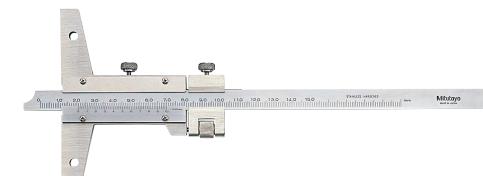

Code number

527-101 527-102 527-103

2 Names of Components

● Caliper



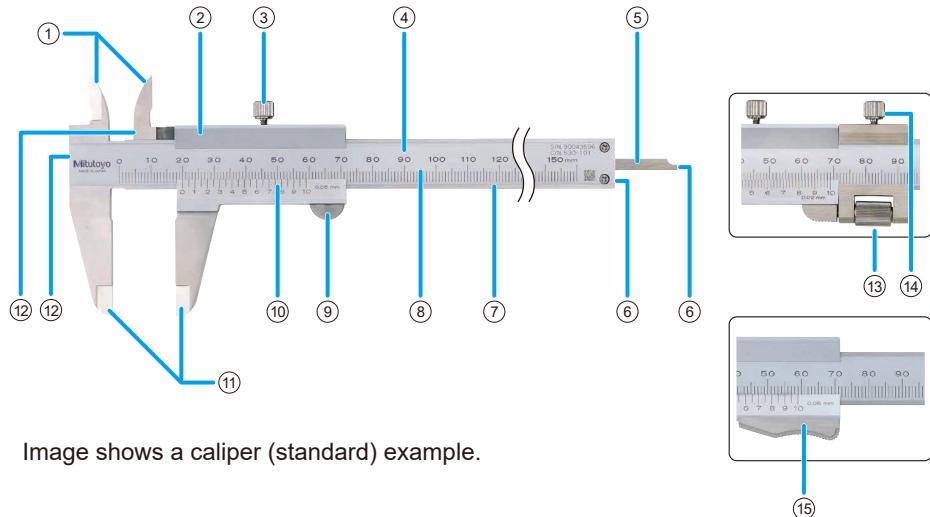


Image shows a caliper (standard) example.

● Caliper (long-size)

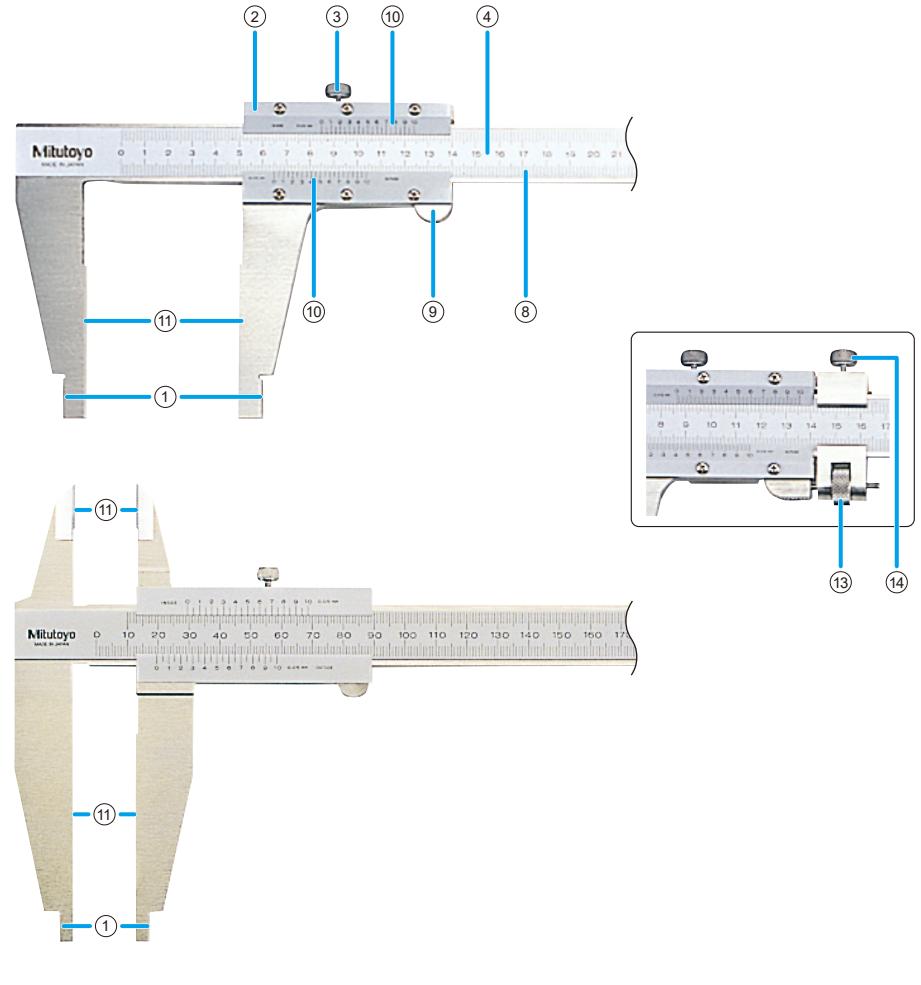

● Depth Gage

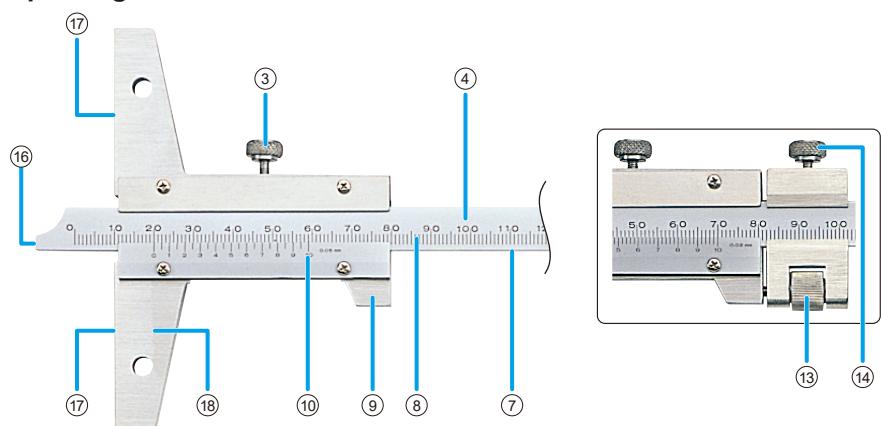


- ① Inside measuring jaws
- ② Slider
- ③ Slider clamp screw
- ④ Beam
- ⑤ Depth bar

- ⑥ Depth measuring faces
- ⑦ Sliding surface (reference surface)
- ⑧ Main scale
- ⑨ Finger rest
- ⑩ Vernier graduation

- ⑪ Outside measuring jaws
- ⑫ Step measuring faces
- ⑬ Fine-adjustment
- ⑭ Fine-adjustment clamp screw
- ⑮ Finger rest (automatic clamp)

- ⑯ Measuring face
- ⑰ Reference surface
- ⑱ Base

3 Product Applications

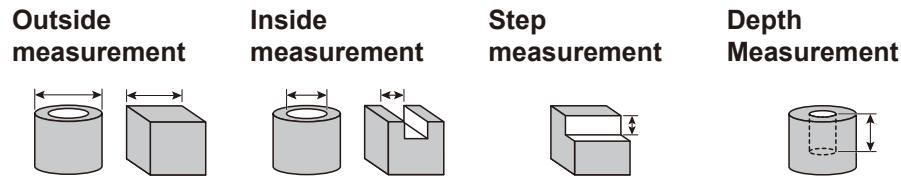

	Outside measurement	Inside measurement	Step measurement	Depth Measurement
Caliper (standard) • With fine-adjustment • With automatic clamp	Yes	Yes	Yes	Yes
Caliper (long-size)	Yes	Yes	No	No
Depth gage	No	No	No	Yes

4 Precautions before Use

- Before using this product for the first time, wipe the rust preventive oil from the product with a soft cloth soaked with cleaning oil. If the rust preventive oil is left on the product, it will dry on and the motion may become stiff. In this case, wipe the sliding surface (reference surface) with a cloth to improve the motion further.
- If cutting chips or debris adhere to the beam, measuring faces, or graduations, wipe them off with chamois or gauze, etc.
- Apply clean oil to the beam, especially the sliding surface. This protects the sliding surface and improves the slider motion.
- Do not perform the adjustment at sites where the temperature will change abruptly. Thermally stabilize the instrument sufficiently at room temperature.

5 Basic Usage

■ Using the caliper/depth gage

For caliper

Grasp the beam lightly with your right hand, put your right thumb on the slider finger rest, and move the slider horizontally to measure.

For depth gage

With one hand, bring the base into close contact with the workpiece, and move the beam vertically with the other hand for measurement.

Tips

- For the measuring method details, refer to "7. Measurement Method".
- For fine-adjustment models, tighten the fine-adjustment clamp and turn the fine-adjustment for fine motion of the slider (caliper) or beam (depth gage).

■ Fixing the slider/base

The main scale and vernier readings are usually taken with the workpiece clamped (or in close contact). However, depending on the measuring location, the orientation during measurement and so on, it may be difficult to get a reading in this position. In this case, tighten the slider clamp screw (caliper) or the clamping screw (depth gage), move the caliper/depth gage carefully away from the workpiece, and read the graduations.

Tips


- For calipers with automatic clamp, the finger rest acts as the automatic clamp. Push the rest in the beam direction to release the clamp and allow the slider to move. Release the rest to fix the slider in that position.

■ Reading the graduations

Read the main scale and vernier graduations from the front.



- There is a slight level difference (H) between the main scale and the vernier. Therefore, if the graduations are read at an angle, parallax will cause measurement error (ΔL).
- If viewing at an oblique angle is unavoidable, we recommend a dial type or digital type without causing parallax.



6 Confirmation before Measurement

■ Confirming Slider Movement

- Confirm that there is no irregular slider movement and that the slider moves smoothly throughout the measurement range.
- Confirm that there is no play of the slider in the vertical direction against the sliding surface.

■ Confirming Main Scale and Vernier Zero Graduation Line Alignment

- For the caliper, close the measuring face of each jaw and confirm that the zero graduation lines are aligned.
- For the depth gage, use a surface plate, etc. to align the measuring face and reference surface, and confirm that the zero graduation lines are aligned.

■ Confirming Clearance (Wear) between Measuring Faces of Caliper


- When the outside measuring jaws are closed and held to the light, confirm that there is no slit observed between the jaws against the light, or that a faint light is uniformly visible. As well, confirm that the jaw tips are not deformed.
- When the inside measuring jaws are closed and held to the light, observing the jaws obliquely, confirm that a light is uniformly visible, and that the tips are not deformed.

7 Measurement Method


■ Precautions when measuring

-  Do not measure the workpiece with the caliper if it is rotating, etc.
Measuring faces will be worn out.
-  The measurement position of long-size vernier calipers should be consistent if positional error is to be avoided. Measurements in vertical positions may differ from those in horizontal positions.

■ Outside measurement

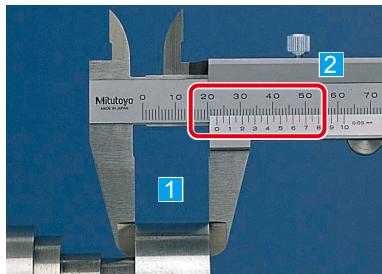


-  • Do not apply excessive force to the workpiece.
Excessive measuring force will cause measurement error because of the positional deviations of the jaws.
- Do not clamp the workpiece diagonally.
Measurement error will ensue if tilted.

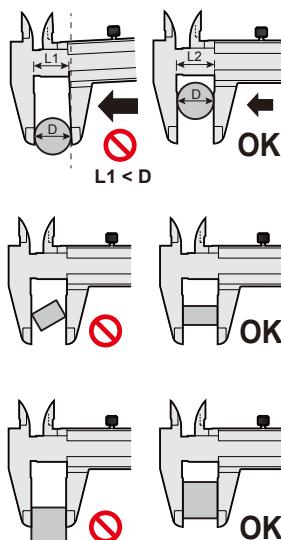


- 1 Insert the workpiece into the outside measuring jaws and bring jaws into close contact with the workpiece, using appropriate and uniform measuring force.
- 2 With the workpiece clamped, read the graduations.

■ Inside measurement

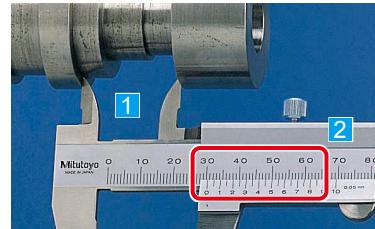


-  • Insert the inside measuring jaws as deeply as possible into the workpiece.

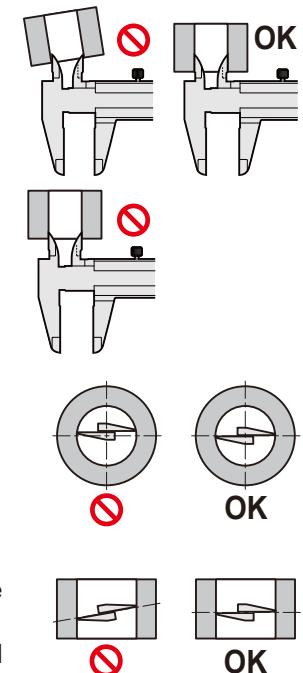


- For inner diameter measurement, bring the measuring faces into close contact, and read the value when the pointer indicated value is maximum: a direct line between the measuring faces passes through the center of the cross-section.
- For groove width measurement, bring the measuring faces into close contact, and read the value when the pointer indicated value is minimum: a direct line between the faces is perpendicular to the groove inner wall.

- 1 Insert the inside measuring jaws into the workpiece, and bring jaws into close contact with the workpiece interior using appropriate and uniform measuring force.
- 2 With the jaws inserted into the workpiece, take the reading.


■ Step measurement

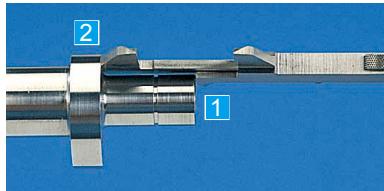

Do not use a depth bar for step measurement, as the small contact area with the workpiece makes it difficult to retain a stable orientation




For a stepped workpiece, bring the entire stepmeasuring surfaces (1, 2) into close contact with the workpiece



- 1 Bring the step measuring face (1, beam side) into close contact with the workpiece.
- 2 Move the slider until the step measuring face (2, slider side) strikes the workpiece (stepped surface).
- 3 With the measuring faces in close contact, take the reading.

■ Depth measurement


For caliper



- 1 For the caliper, bring the depth measuring surface (beam side) into close contact with the workpiece.

For the depth gage, bring the base reference surface into close contact with the workpiece.

The depth measuring face of the caliper is narrow and unstable. Bring it into contact perpendicular with the workpiece.




- 2 For the caliper, move the slider until the depth measuring surface (depth bar side) makes contact.
For the depth gage, move the beam until the measuring face makes contact.
- 3 With the measuring faces in close contact, take the reading.

8 Reading Measurements

The measurement value (C) is obtained by adding the vernier reading (B) that matches the main scale reading (A) shown by the vernier zero graduation line.

■ For resolution: 0.05 mm

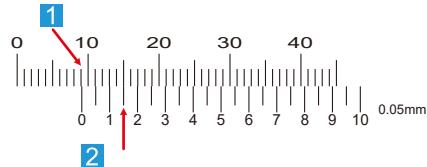

1 Take the main scale reading (A) shown by the vernier zero graduation line.

If the zero graduation line is between two graduations, read the smaller one. For example, if the zero graduation line is between 9 mm and 10 mm, read "9 mm".

$$A = 9 \text{ mm}$$

2 Read the vernier graduation (B) matching the main scale graduation.


For example, if the third vernier graduation line matches the main scale graduation, read "Resolution x graduation = $0.05 \times 3 = 0.15 \text{ mm}$ ".

$$B = 0.05 \text{ mm} \times 3 = 0.15 \text{ mm}$$

3 Add the main scale and vernier readings for the measurement value (C).

$$C = A + B = 9 \text{ mm} + 0.15 \text{ mm} = 9.15 \text{ mm}$$

■ For resolution: 0.02 mm

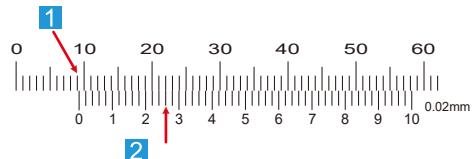

1 Take the main scale reading (A) shown by the vernier zero graduation line.

If the zero graduation line is between two graduations, read the smaller one. For example, if the zero graduation line is between 9 mm and 10 mm, read "9 mm".

$$A = 9 \text{ mm}$$

2 Read the vernier graduation (B) matching the main scale graduation.

For example, if the third vernier graduation line matches the main scale graduation, read "Resolution x graduation = $0.02 \times 13 = 0.26 \text{ mm}$ ".


$$B = 0.02 \text{ mm} \times 13 = 0.26 \text{ mm}$$

3 Add the main scale and vernier readings for the measurement value (C).

$$C = A + B = 9 \text{ mm} + 0.26 \text{ mm} = 9.26 \text{ mm}$$

Tips

For those vernier calipers with a compensation value for inside measurement printed on the jaw, the measurement value (C) is obtained by adding the compensation value to the readings.

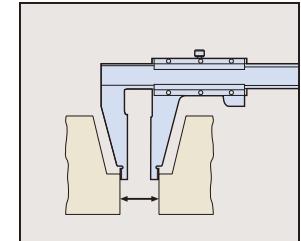

9 Precautions after Use

- If there is dirt on the measuring face, reference surfaces, sliding surface, etc., wipe it away with a dry cloth or a cloth slightly moistened with alcohol.
- For long-term disuse, wipe away any dirt carefully and apply a light coating of rust preventive oil before storage.
- Do not store in locations with high temperatures, low temperatures, high humidity, or exposure to direct sunlight.

©2020 Mitutoyo Corporation. All rights reserved.

Mitutoyo Corporation

20-1, Sakado 1-Chome, Takatsu-ku, Kawasaki-shi, Kanagawa 213-8533, Japan

URL: <https://www.mitutoyo.co.jp>

Printed in Japan

MPE (EMPE, SMPE)

530 Series⁻¹, 531 Series⁻¹

0.05 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07
200 < L ≤ 300	±0.08	±0.10
300 < L ≤ 400	±0.09	±0.11

*L (mm)	EMPE (mm)	SMPE (mm)
400 < L ≤ 500	±0.10	±0.12
500 < L ≤ 600	±0.10	±0.12
600 < L ≤ 700	±0.12	±0.14
700 < L ≤ 800	±0.13	±0.15
800 < L ≤ 900	±0.14	±0.16
900 < L ≤ 1000	±0.15	±0.17

0.02 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.02	±0.04
50 < L ≤ 100	±0.03	±0.05
100 < L ≤ 150	±0.03	±0.05
150 < L ≤ 200	±0.03	±0.05
200 < L ≤ 300	±0.04	±0.06

0.05 mm / 1/128 in

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07
200 < L ≤ 300	±0.08	±0.10

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.5/128	±0.5/128
2 < L ≤ 4	±0.5/128	±0.5/128
4 < L ≤ 6	±0.5/128	±0.5/128
6 < L ≤ 8	±0.5/128	±0.5/128
8 < L ≤ 12	±0.5/128	±0.5/128

1/128 in / 0.001 in

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.5/128	±0.5/128
2 < L ≤ 4	±0.5/128	±0.5/128
4 < L ≤ 6	±0.5/128	±0.5/128
6 < L ≤ 8	±0.5/128	±0.5/128
8 < L ≤ 12	±0.5/128	±0.5/128

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.0010	±0.0020
2 < L ≤ 4	±0.0010	±0.0020
4 < L ≤ 6	±0.0010	±0.0020
6 < L ≤ 8	±0.0010	±0.0020
8 < L ≤ 12	±0.0015	±0.0025

0.02 mm / 0.001 in

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.02	±0.04
50 < L ≤ 100	±0.03	±0.05
100 < L ≤ 150	±0.03	±0.05
150 < L ≤ 200	±0.03	±0.05
200 < L ≤ 300	±0.04	±0.06

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.0010	±0.0020
2 < L ≤ 4	±0.0010	±0.0020
4 < L ≤ 6	±0.0010	±0.0020
6 < L ≤ 8	±0.0010	±0.0020
8 < L ≤ 12	±0.0015	±0.0025

532 Series⁻¹

0.02 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.02	±0.04
50 < L ≤ 100	±0.03	±0.05
100 < L ≤ 130 150	±0.03	±0.05
150 < L ≤ 200	±0.03	±0.05
200 < L ≤ 300	±0.04	±0.06

0.02 mm / 0.001 in

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 2	±0.02	±0.04
2 < L ≤ 4	±0.03	±0.05
4 < L ≤ 6 6	±0.03	±0.05
6 < L ≤ 8 8	±0.03	±0.05
8 < L ≤ 12 12	±0.04	±0.06

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.0010	±0.0020
2 < L ≤ 4	±0.0010	±0.0020
4 < L ≤ 6 6	±0.0010	±0.0020
6 < L ≤ 8 8	±0.0010	±0.0020
8 < L ≤ 12 12	±0.0015	±0.0025

- 1 jp SMPE の中に内径測定 (ø5) は含まれません。
 en Inside diameter measurement (ø5) is not included in SMPE.
 de Die Messung des Innendurchmessers (ø5) ist nicht in SMPE enthalten.
 es La medida del diámetro interio (ø5) no está incluida en SMPE.
 fr La mesure du diamètre intérieur (ø5) n'est pas incluse dans SMPE.
 nl Meting van de binnendiameter (ø5) is niet inbegrepen in SMPE.
 it La misurazione del diametro interno (ø5) non è inclusa in SMPE.
 sv Innerdiameternått (ø5) ingår inte i SMPE.
 pt A medição do diâmetro interno (ø5) não está incluída no SMPE.
 cs Měření vnitřního průměru (ø5) není součástí SMPE.
 pl Pomiar średnicy wewnętrznej (ø5) nie jest uwzględniony w SMPE.
 ru Измерение внутреннего диаметра (ø5) не включено в SMPE.
 tr iç çap ölçümü (ø5) SMPE'ye dahil değildir.
 ko 내경 측정 (ø5)은 SMPE에 포함되지 않습니다.
 zh-CN SMPE 中不包括内径测量 (ø5)。
 zh-TW SMPE 中不包括內徑測量 (ø5)。
 th ກາງວັດເສັ້ນກ່າວຍໜູ້ຄຳກາງໃນ (ø5) ໃນຮຽມອູ້ໃນ SMPE
 vi Phép đo đường kính trong (ø5) không được bao gồm trong SMPE.
 ms Ukuran diameter dalam (ø5) tidak termasuk dalam SMPE.
 id Pengukuran diameter dalam (ø5) tidak termasuk dalam SMPE.

533 Series

0.05 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.05	±0.05
50 < L ≤ 100	±0.05	±0.05
100 < L ≤ 200	±0.05	±0.05
200 < L ≤ 300	±0.08	±0.08
300 < L ≤ 400	±0.08	±0.08
400 < L ≤ 500	±0.10	±0.10

*L (mm)	EMPE (mm)	SMPE (mm)
500 < L ≤ 600	±0.10	±0.10
600 < L ≤ 700	±0.12	±0.12
700 < L ≤ 750	±0.12	±0.12
750 < L ≤ 800	±0.15	±0.15
800 < L ≤ 900	±0.15	±0.15
900 < L ≤ 1000	±0.15	±0.15

0.02 mm: 533-503

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.02	±0.02
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 150	±0.03	±0.03
150 < L ≤ 200	±0.03	±0.03
200 < L ≤ 300	±0.04	±0.04

0.02 mm: 533-504, 533-505, 533-506

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.02	±0.02
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 200	±0.03	±0.03
200 < L ≤ 300	±0.03	±0.03
300 < L ≤ 400	±0.04	±0.04
400 < L ≤ 500	±0.05	±0.05

*L (mm)	EMPE (mm)	SMPE (mm)
500 < L ≤ 600	±0.05	±0.05
600 < L ≤ 700	±0.06	±0.06
700 < L ≤ 750	±0.06	±0.06
750 < L ≤ 800	±0.06	±0.06
800 < L ≤ 900	±0.07	±0.07
900 < L ≤ 1000	±0.07	±0.07

534 Series

0.05 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.07	±0.07
50 < L ≤ 100	±0.07	±0.07
100 < L ≤ 200	±0.07	±0.07
200 < L ≤ 300	±0.07	±0.07
300 < L ≤ 400	±0.13	±0.13
400 < L ≤ 500	±0.13	±0.13

0.02 mm

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.04	±0.04
50 < L ≤ 100	±0.04	±0.04
100 < L ≤ 200	±0.04	±0.04
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.06	±0.06
400 < L ≤ 500	±0.06	±0.06

*L (mm)	EMPE (mm)	SMPE (mm)
500 < L ≤ 600	±0.08	±0.08
600 < L ≤ 700	±0.08	±0.08
700 < L ≤ 750	±0.08	±0.08
750 < L ≤ 800	±0.10	±0.10
800 < L ≤ 900	±0.10	±0.10
900 < L ≤ 1000	±0.10	±0.10

0.05 mm / 1/128 in

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.04	±0.04
50 < L ≤ 100	±0.04	±0.04
100 < L ≤ 200	±0.04	±0.04
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.06	±0.06
400 < L ≤ 500	±0.06	±0.06
500 < L ≤ 600	±0.08	±0.08
600 < L ≤ 700	±0.08	±0.08
700 < L ≤ 750	±0.08	±0.08
750 < L ≤ 800	±0.10	±0.10
800 < L ≤ 900	±0.10	±0.10
900 < L ≤ 1000	±0.10	±0.10

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.5/128	±0.5/128
2 < L ≤ 4	±0.5/128	±0.5/128
4 < L ≤ 8	±0.5/128	±0.5/128
8 < L ≤ 12	±0.5/128	±0.5/128
12 < L ≤ 16	±0.5/128	±0.5/128
16 < L ≤ 20	±0.5/128	±0.5/128
20 < L ≤ 24	±1/128	±1/128
24 < L ≤ 28	±1/128	±1/128
28 < L ≤ 30	±1/128	±1/128
30 < L ≤ 32	±1/128	±1/128
32 < L ≤ 36	±1/128	±1/128
36 < L ≤ 40	±1/128	±1/128

0.02 mm / 0.001 in

*L (mm)	EMPE (mm)	SMPE (mm)
0 ≤ L ≤ 50	±0.04	±0.04
50 < L ≤ 100	±0.04	±0.04
100 < L ≤ 200	±0.04	±0.04
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.06	±0.06
400 < L ≤ 500	±0.06	±0.06
500 < L ≤ 600	±0.08	±0.08
600 < L ≤ 700	±0.08	±0.08
700 < L ≤ 750	±0.08	±0.08
750 < L ≤ 800	±0.10	±0.10
800 < L ≤ 900	±0.10	±0.10
900 < L ≤ 1000	±0.10	±0.10

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.0015	±0.0015
2 < L ≤ 4	±0.0015	±0.0015
4 < L ≤ 8	±0.0015	±0.0015
8 < L ≤ 12	±0.0015	±0.0015
12 < L ≤ 16	±0.0025	±0.0025
16 < L ≤ 20	±0.0025	±0.0025
20 < L ≤ 24	±0.0030	±0.0030
24 < L ≤ 28	±0.0030	±0.0030
28 < L ≤ 30	±0.0030	±0.0030
30 < L ≤ 32	±0.0040	±0.0040
32 < L ≤ 36	±0.0040	±0.0040
36 < L ≤ 40	±0.0040	±0.0040

0.001 in

*L (inch)	EMPE (inch)	SMPE (inch)
0 ≤ L ≤ 2	±0.0015	±0.0015
2 < L ≤ 4	±0.0015	±0.0015
4 < L ≤ 8	±0.0015	±0.0015
8 < L ≤ 12	±0.0015	±0.0015
12 < L ≤ 16	±0.0025	±0.0025
16 < L ≤ 20	±0.0025	±0.0025

*L (inch)	EMPE (inch)	SMPE (inch)
20 < L ≤ 24	±0.0030	±0.0030
24 < L ≤ 28	±0.0030	±0.0030
28 < L ≤ 30	±0.0030	±0.0030
30 < L ≤ 32	±0.0040	±0.0040
32 < L ≤ 36	±0.0040	±0.0040
36 < L ≤ 40	±0.0040	±0.0040

*L jp 測定長さ

en Measured length

de Messlänge

es Longitud medida

fr Longueur mesurée

nl Gemeten lengte

it Lunghezza misurata

sv Mätlängd

pt Comprimento medido

cs Měřená délka

pl Długość pomiaru

ru Длина измерения

tr Ölçme uzunluğu

ko 측정 된 길이

zh-CN 实测长度

zh-TW 實測長度

th ความยาวที่ได้มา

vi Chiều dài đo được

ms Panjang yang diukur

id Panjang terukur

160 Series

0.05 mm

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	±0.05
50 < L ≤ 100	±0.05	±0.05
100 < L ≤ 200	±0.05	±0.05
200 < L ≤ 300	±0.08	±0.08
300 < L ≤ 400	±0.09	±0.09
400 < L ≤ 450	±0.10	±0.10

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
450 < L ≤ 500	±0.10	±0.10
500 < L ≤ 600	±0.10	±0.10
600 < L ≤ 700	±0.12	±0.12
700 < L ≤ 800	±0.13	±0.13
800 < L ≤ 900	±0.14	±0.14
900 < L ≤ 1000	±0.15	±0.15

0.02 mm

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.02	±0.02
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 200	±0.03	±0.03
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.04	±0.04
400 < L ≤ 450	±0.05	±0.05

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
450 < L ≤ 500	±0.05	±0.05
500 < L ≤ 600	±0.05	±0.05
600 < L ≤ 700	±0.06	±0.06
700 < L ≤ 800	±0.06	±0.06
800 < L ≤ 900	±0.07	±0.07
900 < L ≤ 1000	±0.07	±0.07

0.02 mm / 0.001 in

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.02	±0.02
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 200	±0.03	±0.03
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.04	±0.04
400 < L ≤ 450	±0.05	±0.05
450 < L ≤ 500	±0.05	±0.05
500 < L ≤ 600	±0.05	±0.05
600 < L ≤ 700	±0.06	±0.06
700 < L ≤ 800	±0.06	±0.06
800 < L ≤ 900	±0.07	±0.07
900 < L ≤ 1000	±0.07	±0.07

*L (inch)	E _{MPE} (inch)	S _{MPE} (inch)
0 ≤ L ≤ 2	±0.0010	±0.0010
2 < L ≤ 4	±0.0010	±0.0010
4 < L ≤ 8	±0.0010	±0.0010
8 < L ≤ 12	±0.0015	±0.0015
12 < L ≤ 16	±0.0015	±0.0015
16 < L ≤ 18	±0.0020	±0.0020
18 < L ≤ 20	±0.0020	±0.0020
20 < L ≤ 24	±0.0020	±0.0020
24 < L ≤ 28	±0.0020	±0.0020
28 < L ≤ 32	±0.0025	±0.0025
32 < L ≤ 36	±0.0025	±0.0025
36 < L ≤ 40	±0.0030	±0.0030

0.001 in / 0.02 mm

*L (inch)	E _{MPE} (inch)	S _{MPE} (inch)
0 ≤ L ≤ 2	±0.0010	±0.0010
2 < L ≤ 4	±0.0010	±0.0010
4 < L ≤ 8	±0.0010	±0.0010
8 < L ≤ 12	±0.0015	±0.0015
12 < L ≤ 16	±0.0015	±0.0015
16 < L ≤ 18	±0.0020	±0.0020
18 < L ≤ 20	±0.0020	±0.0020
20 < L ≤ 24	±0.0020	±0.0020
24 < L ≤ 28	±0.0020	±0.0020
28 < L ≤ 32	±0.0025	±0.0025
32 < L ≤ 36	±0.0025	±0.0025
36 < L ≤ 40	±0.0030	±0.0030

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.02	±0.02
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 200	±0.03	±0.03
200 < L ≤ 300	±0.04	±0.04
300 < L ≤ 400	±0.04	±0.04
400 < L ≤ 450	±0.05	±0.05
450 < L ≤ 500	±0.05	±0.05
500 < L ≤ 600	±0.05	±0.05
600 < L ≤ 700	±0.06	±0.06
700 < L ≤ 800	±0.06	±0.06
800 < L ≤ 900	±0.07	±0.07
900 < L ≤ 1000	±0.07	±0.07

0.001 in

*L (inch)	E _{MPE} (inch)	S _{MPE} (inch)
0 ≤ L ≤ 2	±0.0010	±0.0010
2 < L ≤ 4	±0.0010	±0.0010
4 < L ≤ 8	±0.0010	±0.0010
8 < L ≤ 12	±0.0015	±0.0015
12 < L ≤ 16	±0.0015	±0.0015
16 < L ≤ 18	±0.0020	±0.0020
18 < L ≤ 20	±0.0020	±0.0020
20 < L ≤ 24	±0.0020	±0.0020
24 < L ≤ 28	±0.0020	±0.0020
28 < L ≤ 32	±0.0025	±0.0025
32 < L ≤ 36	±0.0025	±0.0025
36 < L ≤ 40	±0.0030	±0.0030

*L (inch)	E _{MPE} (inch)	S _{MPE} (inch)
18 < L ≤ 20	±0.0020	±0.0020
20 < L ≤ 24	±0.0020	±0.0020
24 < L ≤ 28	±0.0020	±0.0020
28 < L ≤ 32	±0.0025	±0.0025
32 < L ≤ 36	±0.0025	±0.0025
36 < L ≤ 40	±0.0030	±0.0030

*L jp 測定長さ

en Measured length

de Messlänge

es Longitud medida

fr Longueur mesurée

nl Gemeten lengte

it Lunghezza misurata

sv Mätlängd

pt Comprimento medido

cs Méřená délka

pl Długość pomiaru

ru Длина измерения

tr Ölçme uzunluğu

ko 측정 된 길이

zh-CN 实测长度

zh-TW 實測長度

th ความยาวที่วัดได้

vi Chiều dài đo được

ms Panjang yang diukur

id Panjang terukur

536 Series⁻¹

0.05 mm: 536-101, 536-102, 536-103

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07
200 < L ≤ 300	±0.08	±0.10

0.05 mm: 536-121

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07

0.05 mm: 536-142

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
10 ≤ L ≤ 50	-----	±0.12
50 < L ≤ 100	-----	±0.12
100 < L ≤ 150	-----	±0.12
150 < L ≤ 200	-----	±0.12

0.05 mm: 536-146, 536-147, 536-148, 536-149

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	-----	±0.05
50 < L ≤ 100	-----	±0.05
100 < L ≤ 150	-----	±0.05
150 < L ≤ 200	-----	±0.05
200 < L ≤ 300	-----	±0.08

0.05 mm: 536-151, 536-152, 536-161

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	-----
50 < L ≤ 100	±0.05	-----
100 < L ≤ 150	±0.05	-----

0.05 mm: 536-212

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
10 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07

0.05 mm: 536-105, 536-106, 536-107

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	-----	±0.05
50 < L ≤ 100	-----	±0.05
100 < L ≤ 150	-----	±0.05
150 < L ≤ 200	-----	±0.05
200 < L ≤ 300	-----	±0.08

0.05 mm: 536-134, 536-135, 536-136

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07
200 < L ≤ 300	±0.08	±0.10

0.05 mm: 536-145

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	-----	±0.05
50 < L ≤ 100	-----	±0.05
100 < L ≤ 150	-----	±0.05

0.02 mm: 536-171, 536-172

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
10 ≤ L ≤ 50	±0.03	±0.03
50 < L ≤ 100	±0.03	±0.03
100 < L ≤ 150	±0.03	±0.03
150 < L ≤ 200	±0.03	±0.03

0.05 mm: 536-221, 536-222, 536-223

*L (mm)	E _{MPE} (mm)	S _{MPE} (mm)
0 ≤ L ≤ 50	±0.05	±0.07
50 < L ≤ 100	±0.05	±0.07
100 < L ≤ 150	±0.05	±0.07
150 < L ≤ 200	±0.05	±0.07
200 < L ≤ 300	±0.08	±0.10

-1 jp SMPE の中に内径測定 (ø5) は含まれません。

en Inside diameter measurement (ø5) is not included in SMPE.

de Die Messung des Innendurchmessers (ø5) ist nicht in SMPE enthalten.

es La medida del diámetro interio (ø5) no está incluida en SMPE.

fr La mesure du diamètre intérieur (ø5) n'est pas incluse dans SMPE.

nl Meting van de binnendiameter (ø5) is niet ingegeven in SMPE.

it La misurazione del diametro interno (ø5) non è inclusa in SMPE.

sv Innerdiametermått (ø5) ingår inte i SMPE.

pt A medição do diâmetro interno (ø5) não está incluída no SMPE.

cs Měření vnitřního průměru (ø5) není součástí SMPE.

pl Pomiar średnicy wewnętrznej (ø5) nie jest uwzględniony w SMPE.

ru Измерение внутреннего диаметра (ø5) не включено в SMPE.

tr İç çap ölçümü (ø5) SMPE'ye dahil değildir.

ko 내경 측정 (ø5)은 SMPE에 포함되지 않습니다.

zh-CN SMPE 中不包括内径测量 (ø5)。

zh-TW SMPE 中不包括內徑測量 (ø5)。

th ការវัดតុនៅក្នុងការការពាយ (ø5) មិនរាយក្នុង SMPE

vi Phép đo đùa lòng kính trong (ø5) không được bao gồm trong SMPE.

ms Ukuran diameter dalam (ø5) tidak termasuk dalam SMPE.

id Pengukuran diameter dalam (ø5) tidak termasuk dalam SMPE.

*L jp 測定長さ

sv Mätlängd	zh-CN 實測長度
pt Comprimento medido	zh-TW 實測長度
cs Měřená délka	th គារមាត្រាតីត្រូវដោយ
es Longitud medida	vi Chiều dài đo được
fr Longueur mesurée	ms Panjang yang diukur
nl Gemeten lengte	id Panjang terukur
it Lunghezza misurata	

527 Series

jp	デプスゲージの最大許容誤差は、JIS B7518:2018 に従います。
en	Maximum permissible error for the depth gage conforms to JIS B7518:2018.
de	Zulässiger Wert des Gerätefehlers für das Tiefenmaß entspricht JIS B 7518:2018.
es	Valor permitido de error instrumental para los medidores de profundidades conforman con JIS B 7518:2018.
fr	Erreur acceptable de précision pour jauge de profondeur conforme à la norme JIS B 7518:2018.
nl	Toegestane instrument fout voor de dieptemeter voldoet aan JIS B 7518:2018.
it	Il valore ammesso dell'errore strumentale per il calibro di profondità è conforme alle norme JIS B 7518:2018.
sv	Maximal tillåtet visningsfel för djupmått överensstämmer med JIS B 7518:2018.
pt	O erro máximo permitido para o medidor de profundidade está em conformidade com JIS B 7518:2018.
cs	Maximální přípustná chyba pro hloubkoměr odpovídá JIS B 7518:2018.
pl	Maksymalny dopuszczalny błąd dla wysuwki głębokościomierza jest zgodny z JIS B 7518:2018.
ru	Предел допускаемой основной погрешности измерений глубинометров соответствует JIS B 7518:2018.
tr	Derinlik mastarı için izin verilen maksimum hata JIS B 7518:2018'e uygundur.
ko	뎁스 게이지의 기차 허용 값은 , JIS B 7518:2018 에 따릅니다 .
zh-CN	深度卡尺的仪器误差的容许值，符合 JIS B 7518:2018 规定。
zh-TW	關於深度尺的儀器誤差的容許值為根據 JIS B 7518:2018 。
th	ค่าความผิดพลาดสูงสุดที่ยอมรับได้ ของเกจวัดความลึก ตามข้อกำหนด JIS B 7518:2018.
vi	Sai số tối đa cho phép đối với thước đo độ sâu theo tiêu chuẩn JIS B 7518:2018.
ms	Maksimum ralat yang dibenarkan untuk pengukur kedalaman mematuhi JIS B 7518:2018.
id	Kesalahan Maksimal yang diijinkan untuk Depth Gage sesuai dengan JIS B 7518:2018.